




Schematic Flow Diagram – 2 Position Sample Injector

4 Port Internal (Fixed Volume) Injector P Type Valves, All Series

All Valco valves must be properly supported during tightening or loosening of fittings. This is best effected by the use of one wrench to support the valve body while another wrench tightens or loosens the nut.

Never use the valve shaft as a lever while tightening or loosening nuts.

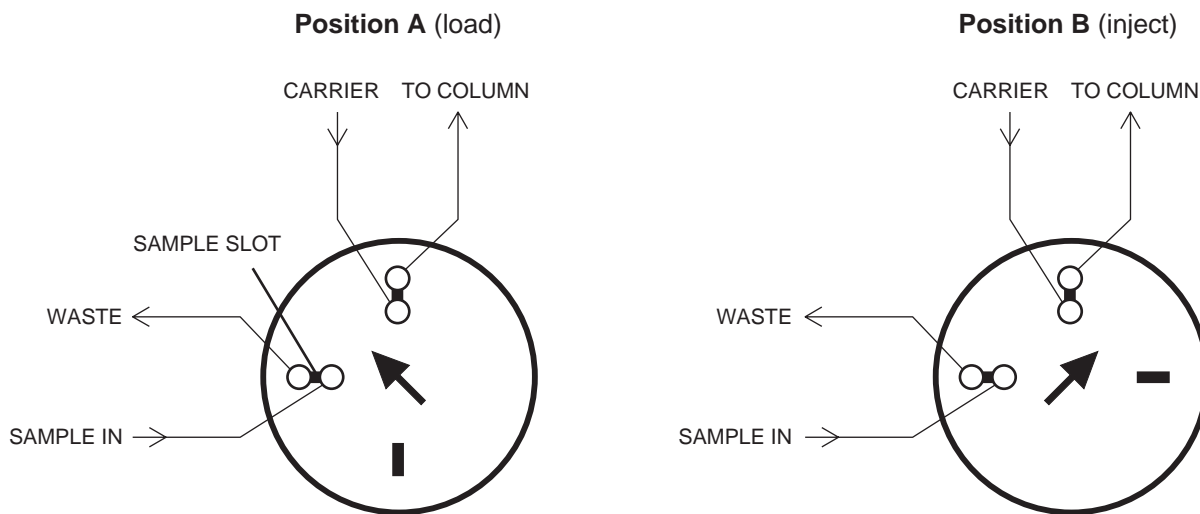

Valve viewed from handle end

Standard sample sizes: 0.2, 0.5, 1.0, 2.0, 3.0, 4.0, and 5.0 μ l

North America, South America, and Australia/Oceania contact:

VICI Valco Instruments Co. Inc.
P.O. Box 55603
Houston, TX 77255
Sales: (800) 367-8424
Tech: (713) 688-9345
Fax: (713) 688-8106 valco@vici.com

Europe, Asia, and Africa contact:

VICI VICI AG International
Parkstrasse 2
CH-6214 Schenkon
Switzerland
Phone: +41 41 925 6200
Fax: +41 41 925 6201 info@vici.ch

Cheminert® and VICI® are registered trademarks of Valco Instruments Co. Inc. and VICI AG

TN-301 10/00